

# Use of End Tidal Oxygen Monitoring to Assess Preoxygenation During Rapid Sequence Intubation in the Emergency Department

Nicholas D. Caputo, MD, MSc\*; Matthew Oliver, MBBS; Jason R. West, MD; Robert Hackett, MBBS; John C. Sakles, MD

\*Corresponding Author. E-mail: [ncaputo.md@gmail.com](mailto:ncaputo.md@gmail.com), Twitter: @NickMD1980.

**Study objective:** Preoxygenation is important to prevent oxygen desaturation during emergency airway management. The purpose of this study is to describe the use of end tidal oxygen (ETO<sub>2</sub>) during rapid sequence intubation in the emergency department.

**Methods:** This study was carried out in 2 academic centers in Sydney, Australia, and New York City. We included patients undergoing rapid sequence intubation in the emergency department. A standard gas analyzer was used to measure ETO<sub>2</sub>. Preoxygenation methods included nonbreather mask and bag-valve-mask ventilation. We measured ETO<sub>2</sub> before preoxygenation and at administration of rapid sequence intubation medications. We also characterized peri-intubation SpO<sub>2</sub>, identifying instances of SpO<sub>2</sub> less than 90%.

**Results:** We included 100 patients during a 6-month period. Median ETO<sub>2</sub> level before and after preoxygenation was 53% (interquartile range [IQR] 43% to 65%) and 78% (IQR 64% to 86%), respectively. One fourth of patients achieved an ETO<sub>2</sub> level greater than 85%. Median ETO<sub>2</sub> level achieved varied with preoxygenation method, ranging from 80% (IQR 60% to 87%) for the nonbreather mask group to 77% (IQR 65% to 86%) for the bag-valve-mask group. The method with the highest median ETO<sub>2</sub> level was nonbreather mask at flush rate (86%; IQR 80% to 90%) and the lowest median ETO<sub>2</sub> level was nonbreather mask at 15 L/min (57%; IQR 53% to 60%). Eighteen patients (18%) experienced oxygen desaturation (SpO<sub>2</sub> <90%); of these, 14 (78%) did not reach an ETO<sub>2</sub> level greater than 85% at induction.

**Conclusion:** ETO<sub>2</sub> varied with different preoxygenation techniques employed in the emergency department. Most patients undergoing rapid sequence intubation did not achieve maximal preoxygenation. Measuring ETO<sub>2</sub> in the emergency department may be a valuable adjunct for optimizing preoxygenation during emergency airway management. [Ann Emerg Med. 2019;■:1-6.]

Please see page XX for the Editor's Capsule Summary of this article.

0196-0644/\$-see front matter

Copyright © 2019 by the American College of Emergency Physicians.

<https://doi.org/10.1016/j.annemergmed.2019.01.038>

## INTRODUCTION

### Background

Rapid sequence intubation is the most common method of airway management in the emergency department (ED).<sup>1</sup> Use of an induction agent and a neuromuscular-blocking agent results in transient apnea during the intubation attempt. If prolonged, apnea and resulting oxygen desaturation may lead to serious adverse events such as dysrhythmias, hypotension, and cardiac arrest.<sup>2</sup> Although practice guidelines advocate preoxygenation to prevent oxygen desaturation, the adequacy of preoxygenation is not typically assessed in the ED.<sup>3-5</sup>

### Importance

In the operating room, anesthesiologists have used gas analyzers to quantify and optimize preoxygenation.<sup>6,7</sup> The

Difficult Airway Society suggests that when critically ill patients are intubated, preoxygenation should be performed until an ETO<sub>2</sub> level of greater than or equal to 85% is attained.<sup>5,8</sup> ETO<sub>2</sub> level has not been widely used in clinical practice in the ED.

### Goals of This Investigation

We sought to describe our preliminary use of ETO<sub>2</sub> to assess preoxygenation during rapid sequence intubation in the ED.

### Study Design and Setting

We conducted a prospective observational cohort study at 2 urban, academic EDs in Sydney, Australia, and New York City. This study was approved with waiver of consent by the institutional review board and ethics boards at each institution.

**Editor's Capsule Summary***What is already known on this topic*

Preoxygenation is recommended before rapid sequence intubation.

*What question this study addressed*

Can end tidal expired oxygen levels (ETO<sub>2</sub>) characterize preoxygenation before rapid sequence intubation?

*What this study adds to our knowledge*

In this series of 100 rapid sequence intubations, median ETO<sub>2</sub> levels before and after preoxygenation were 53% (interquartile range 43% to 65%) and 78% (interquartile range 64% to 86%). Of the 18 patients experiencing oxygen desaturation (SaO<sub>2</sub> <90%), 14 (78%) had an ETO<sub>2</sub> level less than 85% before induction.

*How this is relevant to clinical practice*

ETO<sub>2</sub> level may be useful for guiding preoxygenation during rapid sequence intubation in the ED. However, formal validation is necessary before clinical implementation.

The annual census of each ED was 175,000 patients (New York) and 80,000 patients (Sydney). The departments perform greater than 900 intubations a year combined (approximately 300 at the Sydney site and 600 at the New York site). Each department has emergency medicine trainees. The majority of intubations are performed by emergency medicine trainees under the direct supervision of an emergency medicine attending physician. Both sites practice rapid sequence intubation, with the specific technique used chosen by the emergency medicine attending physician.

Clinical airway management practices at each site called for a minimum of 3 minutes of preoxygenation with either a bag-valve-mask device or a nonrebreather mask before rapid sequence intubation. If a bag-valve-mask device was used, the mask seal was maintained by the operator, and assisted breaths were given at the discretion of the attending physician. Positive end-expiratory pressure could be provided if clinically warranted by means of a positive end-expiratory pressure valve connected to the bag-valve-mask device, and at pressures ranging from 1 to 20 cm H<sub>2</sub>O. For nonrebreather mask, the oxygen flow rate was selected by the emergency medicine attending physician and was set at either 15 L/min or flush rate (50 to 70 L/min at the New York site and 19 L/min at the Sydney site). The use of

supplemental nasal cannula oxygen was chosen by the attending emergency physician and ranged from 15 L/min to flush rate.

**Selection of Participants**

We included all adult patients (≥18 years) undergoing rapid sequence intubation during October 2017 to February 2018. We excluded patients in cardiac arrest, receiving noninvasive ventilation before intubation, intubated in the out-of-hospital setting, or who underwent awake intubation.

**Methods of Measurement**

To quantify ETO<sub>2</sub> level achieved with current preoxygenation practices, emergency physicians were blinded to the ETO<sub>2</sub> data collected during the procedure. Independent observers (research assistants, nurses, and residents) collected all ETO<sub>2</sub> measurements. The observers underwent training for the study and collected data in real time, using a standardized data collection tool.

Vital signs were obtained from the cardiac monitor (Philips IntelliVue; Philips, Andover, MA) in real time. ETO<sub>2</sub> level was measured by Phillips G5 Gas Analyzer (Philips) at the New York site and by a Philips G7 Gas Analyzer (Philips) at the Sydney site. The newer-generation G7 module is a more compact version of the G5 and facilitates similar ETO<sub>2</sub> measurements. Although not the focus of this study, the devices also measured FiO<sub>2</sub>. The analyzers use a single flow sensor to make measurements for FiO<sub>2</sub> supplied and ETO<sub>2</sub> exhaled by gas sampling. SpO<sub>2</sub> was measured through standard finger oximeters (Covidien Oximax; Covidien). Hypoxemia was defined as an SpO<sub>2</sub> level less than 90%.

For patients undergoing bag-valve-mask preoxygenation, ETO<sub>2</sub> level was measured by side-stream gas sampling connected between the bag-valve-mask device and the mask. For patients receiving nonrebreather mask preoxygenation, side-stream sampling was used by means of a nasal prong gas sampler (AirLife ETCO<sub>2</sub> Nasal Cannula at the New York site and CapnoEZY at the Sydney site). For patients receiving preoxygenation by nonrebreather mask plus nasal cannula oxygen, the New York site used a separate standard nasal cannula. The Sydney site used CapnoEZY nasal prongs. Waveform capnography was used to verify that ventilation was occurring during ETO<sub>2</sub> measurement recordings.

To validate the use of single-breath versus continuous ETO<sub>2</sub> measurements, we conducted a preliminary study using 4 healthy volunteers (attaining 20 measurements at each site). We compared continuous and single-breath ETO<sub>2</sub> measurements for both bag-valve-mask device and

nonbreather mask (n=10 measurements for each method). Each volunteer was preoxygenated for 3 minutes with bag-valve-mask device and nonbreather mask. The  $ETO_2$  was recorded at the end of 3 minutes of continuous analysis. At the conclusion of the 3 minutes, the subject held a single breath for 10 seconds and then exhaled. This single-breath measurement was then compared with the final measurement during the continuous  $ETO_2$  measurement.

Preoxygenation interval was defined as the elapsed time from emergency medicine attending physician decision to intubate to the point of induction. Apnea time was defined as the elapsed time from induction to confirmation of tube placement by waveform capnography. All other data on baseline characteristics, pre- and postlaryngoscopy management, and clinical outcomes were collected from the medical record by study personnel. We tested interrater agreement for  $ETO_2$  and  $SpO_2$  by using the first 5 cases.

### Outcome Measures

The primary outcome was  $ETO_2$  level, measured before preoxygenation and at induction. The secondary outcome was  $SpO_2$ , measured before and immediately after intubation.

### Primary Data Analysis

To validate the use of single-breath versus continuous  $ETO_2$  in healthy volunteers, we used Pearson's correlation coefficient and a Bland-Altman plot. For the clinical series, we analyzed the data with descriptive techniques. We determined median  $ETO_2$  level before preoxygenation and at induction, and  $SpO_2$  before and after intubation, examining the full cohort, as well as stratifying by preoxygenation technique. We plotted  $ETO_2$  and  $SpO_2$  measurements for each patient. We determined the proportion of patients achieving  $ETO_2$  level greater than 85%. We also determined the proportion of patients who experienced oxygen desaturation ( $SpO_2 < 90\%$ ). For the initial 5 subjects, we assessed percentage agreement between raters. All analyses were performed with XLStat (version 2018.7; Addinsoft, New York, NY).

## RESULTS

In the validation of continuous versus single-breath  $ETO_2$  measurements using human volunteers, continuous  $ETO_2$  level for the bag-valve-mask group was 82% (95% confidence interval [CI] 80% to 86%) and single-breath  $ETO_2$  was 80% (95% CI 74% to 86%); the mean difference was 2.2% (95% CI 1.4% to 3%) for the bag-valve-mask group. Continuous  $ETO_2$  level for the nonbreather mask

group was 70% (95% CI 62% to 78%) for continuous  $ETO_2$ , and single-breath  $ETO_2$  was 75% (95% CI 68% to 82%); the mean difference was 5% (95% CI 3.5% to 6.5%) for the nonbreather mask group. Agreement was good between the measures with Pearson's correlation coefficient 0.81 (95% CI 0.59 to 0.92) for the bag-valve-mask device and 0.75 (95% CI 0.45 to 0.90) for nonbreather mask (Bland-Altman plot depicted in [Figure E1](#), available online at <http://www.annemergmed.com>).

Of 154 patients undergoing rapid sequence intubation, we included 100, including 75 at the New York site and 25 at the Sydney site. Reasons for exclusion included the following: noninvasive ventilation before intubation (n=18), intubation in the field (n=11), use of "awake" intubation (n=13), and traumatic cardiac arrest (n=3). Data were not available for 9 patients. The cohort was composed of older patients, greater than half of whom were men, with a primary indication for intubation that was pulmonary at the New York site and neurologic at the Sydney site ([Table](#)). Video laryngoscopy was used for 55% of patients at the New York site (data not collected at the Sydney site), and senior trainees intubated 65% of the patients. The first-pass success was 90% and all patients were intubated within 2 attempts.

For the first 5 consecutively included patients, interrater agreement was high for  $ETO_2$  (percentage agreement=80%) and  $SpO_2$  (percentage agreement=100%) before preoxygenation and at rapid sequence intubation induction.

The median  $ETO_2$  level at initiation of preoxygenation was 53% (interquartile range [IQR] 43% to 65%) and at induction was 78% (IQR 64% to 86%). The median  $ETO_2$  levels for the nonbreather mask and the bag-valve-mask device subgroups were similar at induction (80%, IQR 59% to 87%; and 77%, IQR 65% to 86%, respectively). The method with the highest median  $ETO_2$  level was nonbreather mask at flush rate (86%; IQR 80% to 90%), and the lowest median  $ETO_2$  level was nonbreather mask at 15 L/min (57%; IQR 53% to 60%). The median  $FiO_2$  at induction was 90% (IQR 78% to 94%). The mean  $SpO_2$  at induction was 97% (95% CI 93% to 99%). Oxygen saturations were higher during rapid sequence intubation when higher  $ETO_2$  levels were achieved by induction ([Figure](#)). Only approximately a quarter of the patients achieved an  $ETO_2$  level greater than 85% (n=26). Of 100 patients, 36 (36%) were able to be preoxygenated to an  $ETO_2$  level of 70% to 85%, and 27 (27%) to an  $ETO_2$  level of 50% to 69%. A total of 11 patients (11%) did not achieve an  $ETO_2$  level greater than 50%; the majority were in the bag-valve-mask group.

**Table.** Baseline characteristics of the overall cohort.

| Characteristic                             | Site 1<br>(n = 75) | Site 2<br>(n = 25) | Total Cohort<br>(N = 100) |
|--|--------------------|--------------------|---------------------------|
| Age, median (IQR), y                       | 57                 | 41                 | 53                        |
| Male sex, No. (%)                          | 50                 | 60                 | 56                        |
| <b>Indication, No. (%)</b>                 |                    |                    |                           |
| Pulmonary                                  | 36                 | 1                  | 37 (37)                   |
| Neurologic                                 | 18                 | 7                  | 25 (25)                   |
| Trauma                                     | 14                 | 5                  | 19 (19)                   |
| Infections (not including pulmonary)       | 1                  | 6                  | 7 (7)                     |
| Other                                      | 6                  | 6                  | 12 (12)                   |
| <b>Preoxygenation method, No. (%)</b>      |                    |                    |                           |
| BVM at 15 L/min                            | 7                  | 6                  | 12 (12)                   |
| BVM at FR                                  | 17                 | 0                  | 17 (17)                   |
| BVM+PEEP at 15 L/min                       | 4                  | 8                  | 13 (13)                   |
| BVM+PEEP at FR                             | 13                 | 0                  | 13 (13)                   |
| NRB at 15 L/min                            | 9                  | 3                  | 12 (12)                   |
| NRB at FR                                  | 17                 | 0                  | 17 (17)                   |
| NRB+NC at 15 L/min                         | 4                  | 8                  | 12 (12)                   |
| NRB+NC at FR                               | 4                  | 0                  | 4 (4)                     |
| <b>Timing</b>                              |                    |                    |                           |
| Preoxygenation time, median (IQR), min     | 12 (11 to 15)      | 11 (8 to 14)       | 12 (10 to 14)             |
| <b>Operator level of training, No. (%)</b> |                    |                    |                           |
| <b>PGY</b>                                 |                    |                    |                           |
| 1  | 11                 | 0                  | 8                         |
| 2  | 36                 | 0                  | 27                        |
| ≥3   | 53                 | 100                | 65                        |

BVM, Bag-valve-mask; PEEP, positive end-expiratory pressure; NRB, nonrebreather mask; FR, flush rate (ie, 50 to 70 L/min); NC, nasal cannula; PGY, postgraduate year.

A total of 18 patients (18%) desaturated below 90%, and 2 (2%) desaturated below 80%. Of these 18 patients, 2 (11%) had an  $ET_{O_2}$  level greater than 85% at rapid sequence intubation induction; the remaining cases had  $ET_{O_2}$  level less than 85% at induction.

## LIMITATIONS

There are several limitations to this study. The study centers were academic EDs with training programs, and thus the results may not generalize to nonacademic centers. Because of the preliminary nature of this study, we did not compare differing techniques nor associations with patient outcomes or adverse events (dysrhythmia, hypotension, and cardiac arrest). Although this was a limitation, we believed it was necessary to determine the foundation of whether an

issue existed with current preoxygenation strategies or techniques in the ED by means of measuring  $ET_{O_2}$ . Although our validation of continuous monitoring demonstrated results similar to those of a single breath technique, they were not identical, so caution needs to be taken. The type of monitoring technique may have limitations on accuracy because there is a potential for a difference between single-breath and continuous  $ET_{O_2}$  measurements. The  $ET_{O_2}$  results of continuous measuring may be slightly higher than single-breath measurements in critically ill patients because of oxygen mixing from the source in the mask when the patient is not ventilating adequately, which does not occur during a single-breath measurement. In critically ill patients, it is difficult to control for tidal volume breathing before securing an airway, and therefore mixing may take place at times.

$ET_{O_2}$  represents only a measure of the concentration of oxygen in the functional reserve capacity. Critically ill patients may achieve a very high  $ET_{O_2}$  but have a short safe apnea time because of a markedly reduced functional reserve capacity, increased oxygen consumption, or both.<sup>9</sup>  $ET_{O_2}$  measurements can be inaccurate if proper technique is not used. For example, in a patient with severe hypoventilation the oxygen analyzer would essentially measure the  $FiO_2$  being delivered to the patient.<sup>10</sup> The concurrent use of waveform analysis (of both carbon dioxide and oxygen) is vital to determine alveolar gas exchange.


Although our gas analyzer devices were able to measure  $FiO_2$ , we limited inferences on this measure because of inherent technical limitations with this technique; for example, if a patient receiving nonrebreather mask is not ventilating well, the supplemental oxygen may concentrate in the mask, causing falsely elevated  $FiO_2$ . If validated, measured  $FiO_2$  could offer another tool for monitoring and enhancing preoxygenation.

## DISCUSSION

In this observational study, we describe our experience with using  $ET_{O_2}$  as a means of quantifying the adequacy of current preoxygenation strategies in the ED.  $ET_{O_2}$  use must be formally validated before its widespread use in the ED setting. However, this technology could provide an additional tool to guide clinical care during emergency airway management.

Denitrogenation of the functional reserve capacity with oxygen is a vital step in preoxygenation before intubation to create an intrapulmonary reservoir of oxygen that prevents hypoxemia during the apneic phase of intubation. Gas analysis monitoring of  $ET_{O_2}$  results has been used in the operating room for decades to help guide clinicians on the



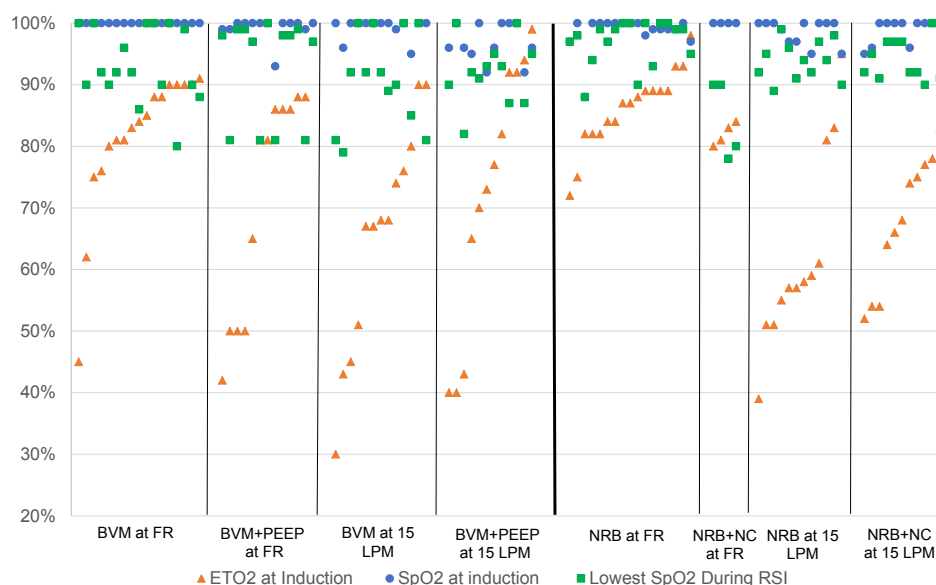

**Figure.** Induction  $ETO_2$ , induction  $SpO_2$ , and lowest  $SpO_2$  measurement for each rapid sequence intubation patient. LPM, Liters per minute; RSI, rapid sequence intubation.

effectiveness of denitrogenation before a patient undergoes anesthesia for operative intervention.<sup>10,11</sup> These analyzers provide useful information that can be used to adjust in real time the method of preoxygenation being used, adjust what flow rate is being used, determine whether there is good mask seal, and determine whether these adjustments make a difference. Historically, EDs have not routinely used gas analyzers for  $ETO_2$ , likely because of the lack of access to the technology, high costs, and unfamiliarity with the device and technique. Although rapid sequence intubation in the ED includes the preoxygenation phase of patients, because the procedure is generally considered to be deemed emergency, this may reflect less than adequate focus being placed on spending time and resources on optimizing patients, who are already at high risk for desaturation by the nature of their critical illness.<sup>3</sup> Many articles in the emergency medicine literature have emphasized the importance of the preoxygenation of patients, and subsequently clinical practices have changed to optimize patients before intubation.<sup>3,12</sup> This is where the implementation of  $ETO_2$  may have use.

We found that only 26% of patients were able to be preoxygenated to the recommended goal of an  $ETO_2$  level greater than or equal to 85%.<sup>5,8</sup> There are a number of potential causes for low  $ETO_2$  measurements. Low  $FiO_2$  may result from inadequate oxygen flow or leaks in the face mask seal. Also, the time required for denitrogenation varies between patients; 3 minutes may not be sufficient for some patients. In the operating room, Baillard et al<sup>13</sup> found that of 1,050 patients preoxygenated for a set time of 3 minutes with an anesthetic circuit, only 44% achieved

adequate preoxygenation, defined as  $ETO_2$  level greater than or equal to 90%. Given that this study was conducted in the controlled environment of the operating room on elective surgical patients, it perhaps is not surprising that the majority of patients who achieved optimal preoxygenation in our study was so low. Compared with studies on healthy volunteers undergoing preoxygenation, our results appear to be fairly similar.<sup>14-17</sup> This suggests that measuring  $ETO_2$  in critically ill patients is feasible and may be useful to help optimize preoxygenation.

In summary, in this preliminary study we observed considerable variation in  $ETO_2$  level during preoxygenation for ED rapid sequence intubation.  $ETO_2$  may be a useful adjunct to optimize preoxygenation during emergency airway management.

*The authors acknowledge Scott Weingart, MD, and Nicholas Chrimes, MBBS, for advice and guidance throughout the article preparation phase of the study.*

Supervising editor: Henry E. Wang, MD, MS. Specific detailed information about possible conflict of interest for individual editors is available at <https://www.annemergmed.com/editors>.

Author affiliations: From the Department of Emergency Medicine, Lincoln Medical Center, Bronx, NY (Caputo, West); the Department of Emergency Medicine (Oliver) and Department of Anaesthesia (Hackett), Royal Prince Alfred Hospital, University of Sydney, Sydney, Australia; and the Department of Emergency Medicine, University of Arizona College of Medicine, Tucson, AZ (Sakles).

Author contributions: NDC, MO, JRW, RH, and JCS contributed to the research design and methodology, initial drafting, and editing

of the manuscript. NDC, JRW, and MO supervised the data collection. NDC performed the data analysis. NDC takes responsibility for the paper as a whole.

All authors attest to meeting the four [ICMJE.org](http://www.icmje.org) authorship criteria: (1) Substantial contributions to the conception or design of the work; or the acquisition, analysis, or interpretation of data for the work; AND (2) Drafting the work or revising it critically for important intellectual content; AND (3) Final approval of the version to be published; AND (4) Agreement to be accountable for all aspects of the work in ensuring that questions related to the accuracy or integrity of any part of the work are appropriately investigated and resolved.

**Funding and support:** By *Annals* policy, all authors are required to disclose any and all commercial, financial, and other relationships in any way related to the subject of this article as per ICMJE conflict of interest guidelines (see [www.icmje.org](http://www.icmje.org)). The authors have stated that no such relationships exist.

**Publication dates:** Received for publication December 12, 2018. Revisions received January 6, 2019, and January 21, 2019. Accepted for publication January 22, 2019.

Presented at the American College of Emergency Physicians national *Scientific Assembly*, October 2018, San Diego, CA; and the New York Chapter of American College of Emergency Physicians regional *Scientific Assembly*, July 2018, Lake George, NY.

## REFERENCES

1. Brown CA 3rd, Bair AE, Pallin DJ, et al; NEAR III Investigators. Techniques, success, and adverse events of emergency department adult intubations. *Ann Emerg Med.* 2015;65:363-370.
2. Heffner AC, Swords DS, Neale MN, et al. Incidence and factors associated with cardiac arrest complicating emergency airway management. *Resuscitation.* 2013;84:1500-1504.
3. Weingart SD, Levitan RM. Preoxygenation and prevention of desaturation during emergency airway management. *Ann Emerg Med.* 2012;59:165-175.
4. Tanoubi I, Drolet P, Donati F. Optimizing preoxygenation in adults. *Can J Anaesth.* 2009;56:449-466.
5. Frerk C, Mitchell VS, McNarry AF, et al. Difficult Airway Society Intubation Guidelines Working Group. Difficult Airway Society 2015 guidelines for management of unanticipated difficult intubation in adults. *Br J Anaesth.* 2015;115:827-848.
6. Benumof JL. Preoxygenation: best method for both efficacy and efficiency. *Anesthesiology.* 1999;91:603-605.
7. Pourmand A, Robinson C, Dorwart K, et al. Pre-oxygenation: implications in emergency airway management. *Am J Emerg Med.* 2017;35:1177-1183.
8. Higgs A, McGrath BA, Goddard C, et al. Difficult Airway Society; Intensive Care Society; Faculty of Intensive Care Medicine; Royal College of Anaesthetists. Guidelines for the management of tracheal intubation in critically ill adults. *Br J Anaesth.* 2018;120:323-352.
9. Benumof JL, Herway ST. High end-tidal oxygen concentration can be a misleading sole indicator of the completeness of preoxygenation. *Anesth Analg.* 2017;124:2093.
10. American Society of Anesthesiologists. Standards for basic anesthetic monitoring, October 15, 2003. Available at: <http://www.asahq.org/publicationsAndServices/standards/02.pdf#2>. Accessed August 2, 2018.
11. Australia and New Zealand College of Anaesthetists. Recommendations on monitoring during anaesthesia, October 2000. Available at: [http://www.medeserv.com.au/anzca/publications/profdocs/profstandards/PS18\\_2000.htm](http://www.medeserv.com.au/anzca/publications/profdocs/profstandards/PS18_2000.htm). Accessed September 26, 2004.
12. Sakles JC. Maintenance of oxygenation during rapid sequence intubation in the emergency department. *Acad Emerg Med.* 2017;24:1395-1404.
13. Baillard C, Depret F, Levy V, et al. Incidence and prediction of inadequate preoxygenation before induction of anaesthesia. *Ann Fr Anesth Reanim.* 2014;33:e55-e58.
14. Driver BE, Prekker ME, Kornas RL, et al. Flush rate oxygen for emergency airway preoxygenation. *Ann Emerg Med.* 2017;69:1-6.
15. Driver BE, Klein LR, Carlson K, et al. Preoxygenation with flush rate oxygen: comparing the nonrebreather mask with the bag-valve mask. *Ann Emerg Med.* 2018;71:381-386.
16. Hayes-Bradley C, Lewis A, Burns B, et al. Efficacy of nasal cannula oxygen as a preoxygenation adjunct in emergency airway management. *Ann Emerg Med.* 2016;68:174-180.
17. Groombridge C, Chin CW, Hanrahan B, et al. Assessment of common preoxygenation strategies outside of the operating room environment. *Acad Emerg Med.* 2016;23:342-346.